

	Fiche machine n°	<h1>Autoclave</h1>	FRM-007
	5879		Indice A
	Indice A		Page 1 / 20

Autoclave

Fabricant : BOSCH SBM

Année : 1990

Reconditionné en 2010 (chambre et tuyauterie) et 2014 (automatisme)

Type : mixte air-vapeur

Volume : 2510 L

Température max : 150 °C

Pression max : 3 / -1 bar

Stérilisateur Turbotherm SDT-13.09.15/2

Chariots et plateaux présents

GVP présent

Incoterm : EXW

Autoclave

Manufacturer: BOSCH SBM

Year: 1990

Refurbished in 2010 (chamber and pipes) and 2014 (automatism)

Type: combined air-steam

Volume: 2510 L

Max temperature: 150 °C

Max pressure: 3 / -1 bar

Turbotherm sterilizer SDT-13.09.15/2

Trolleys and trays available

PSG available

Incoterm: EXW

Autoclave











Autoclave







SBM

SCHOELLER-BLECKMANN
M E D I Z I N T E C H N I K




**Local
technique**









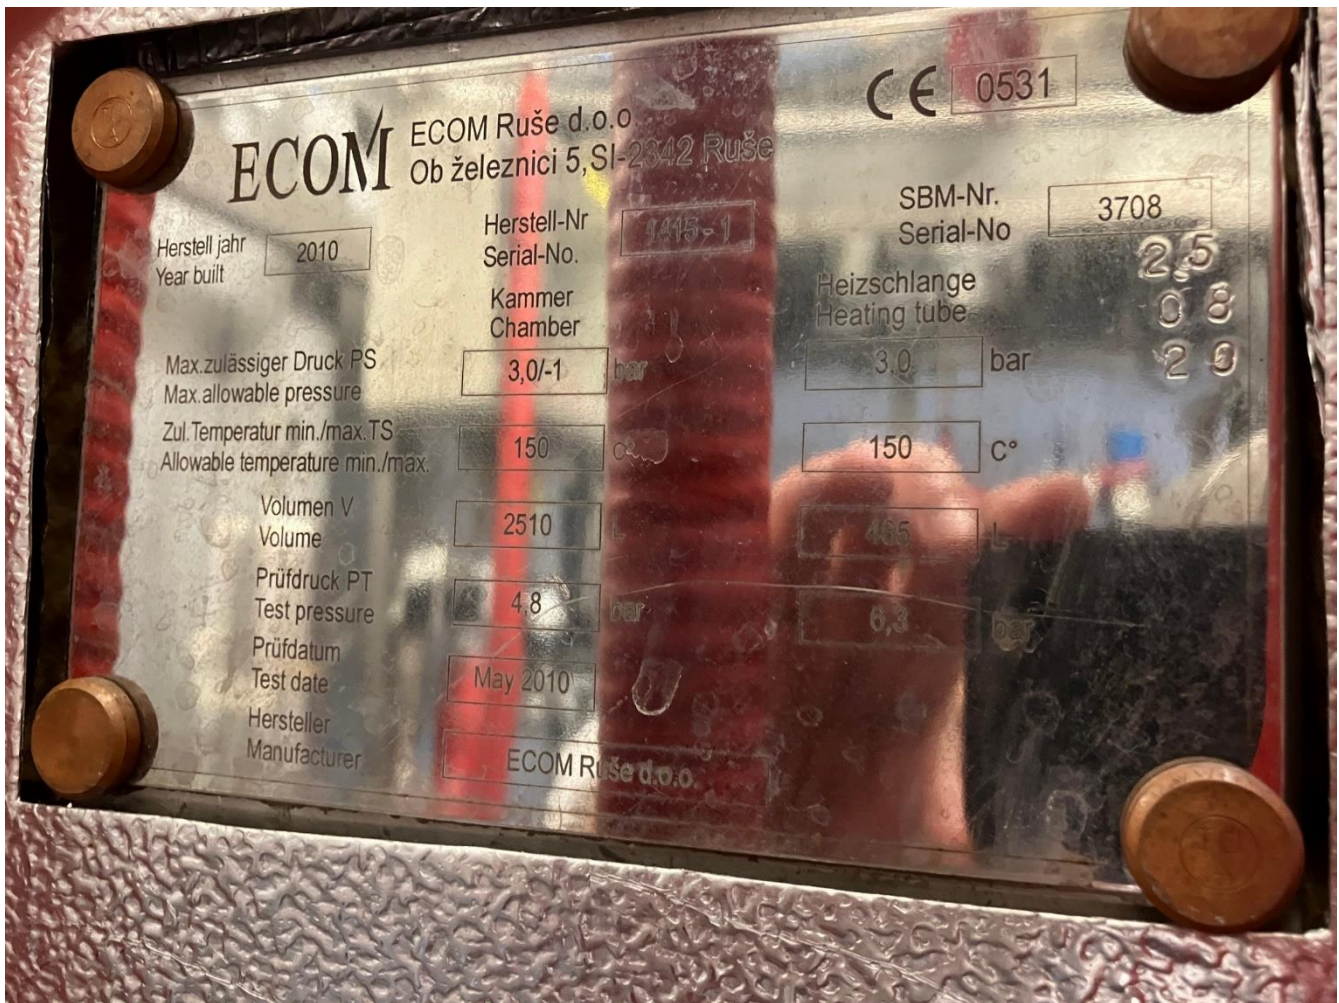

Autoclave





Equipment Documentation

Catalent France
France

SDT-13.09.15/2
TURBOTHERM - STERILIZER



BOSCH

Year of construction
1990

Upgrade 2010 + 2014

Machine no./ Plant no.

SBM FA: 3708 (3050)

Overall order no.

SBM SCHOELLER-BLECKMANN MEDIZINTECHNIK Ges.m.b.H.
A BOSCH Packaging Technology Company
Pharmastrasse 1
A - 2630 Ternitz
Austria

Phone: ++43 2630 312 - 0
Fax: ++43 2630 35947
E-Mail: sales.sbm@bosch.com
www.boschpackaging.com

© Robert Bosch GmbH

All rights reserved, also regarding any disposal, exploitation, reproduction, editing, distribution, as well as in the event of applications for industrial property rights.
These documents are the property of Robert Bosch GmbH and are to be produced nor made known to a third party without our written approval.

Autoclave

